

FIG. 1

PRIOR ART

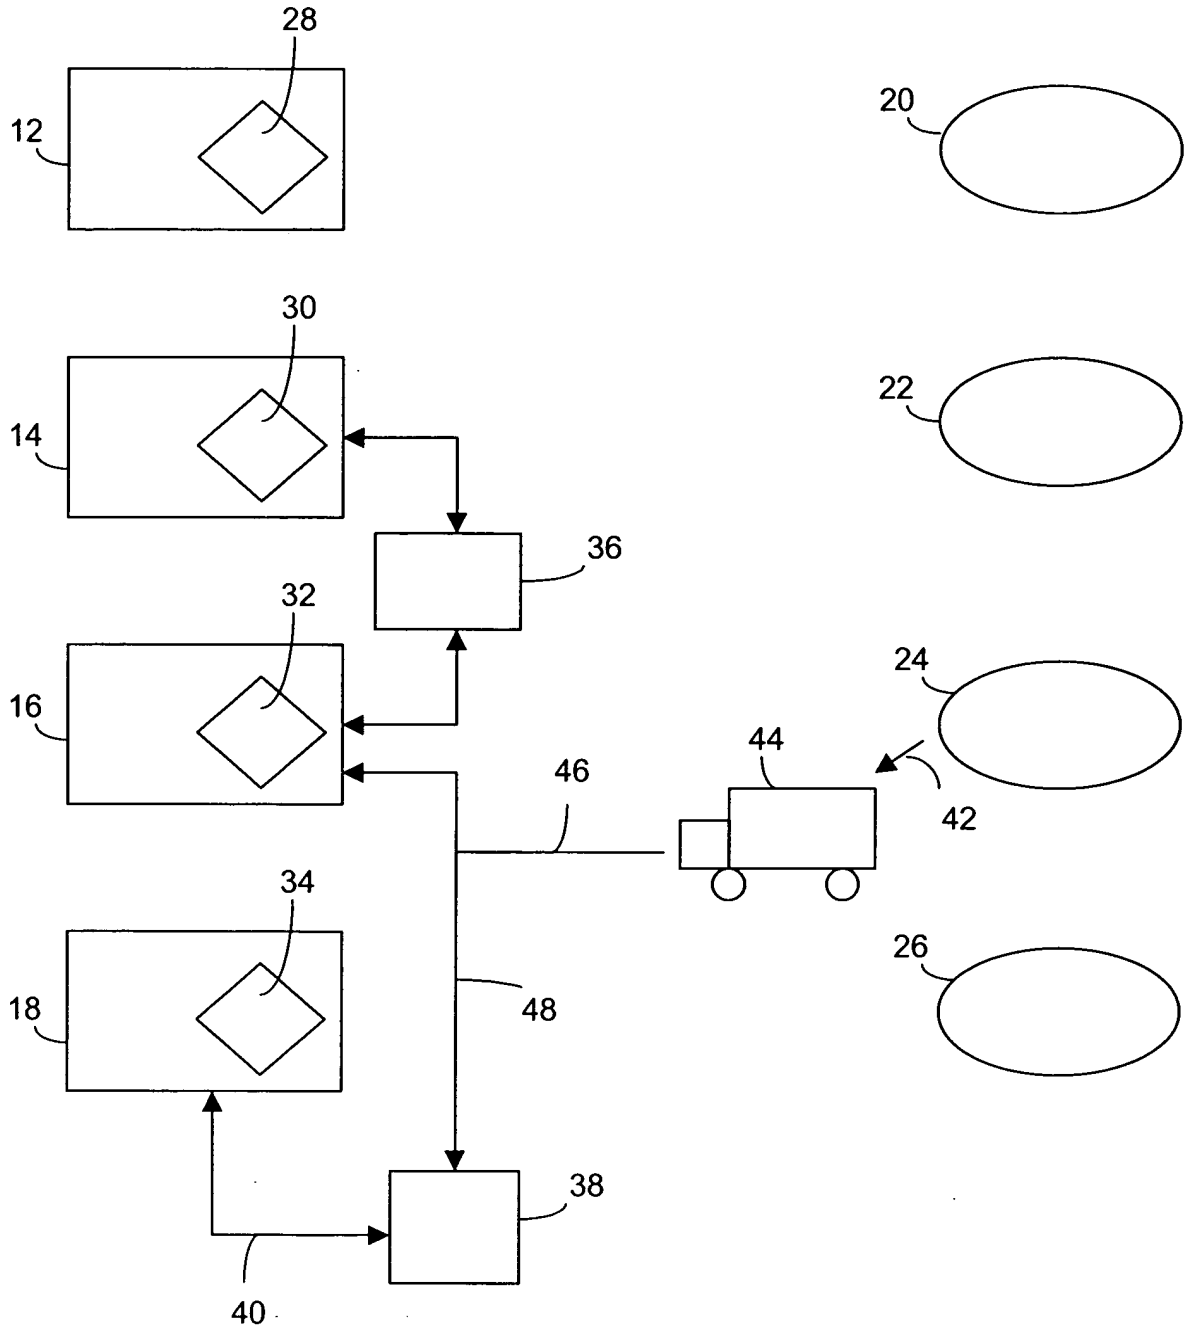
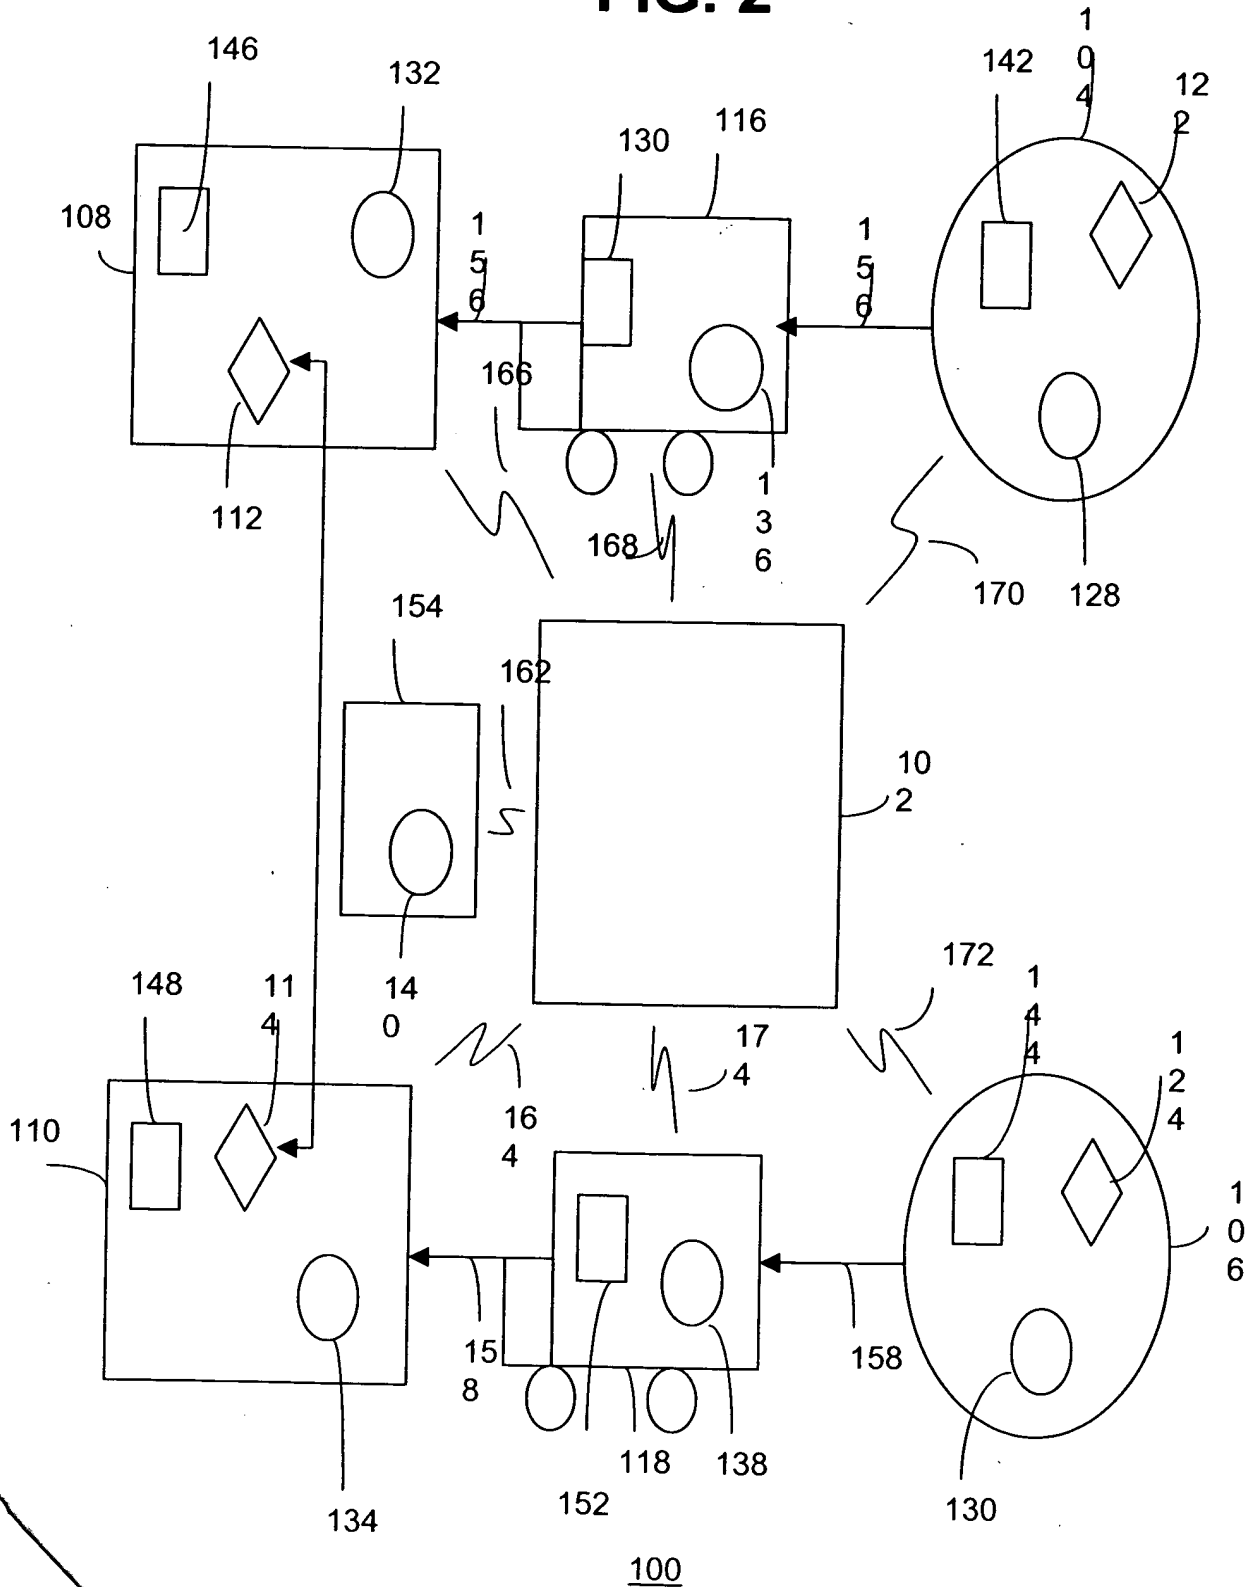


FIG. 2



2004-03-03 10:30:00

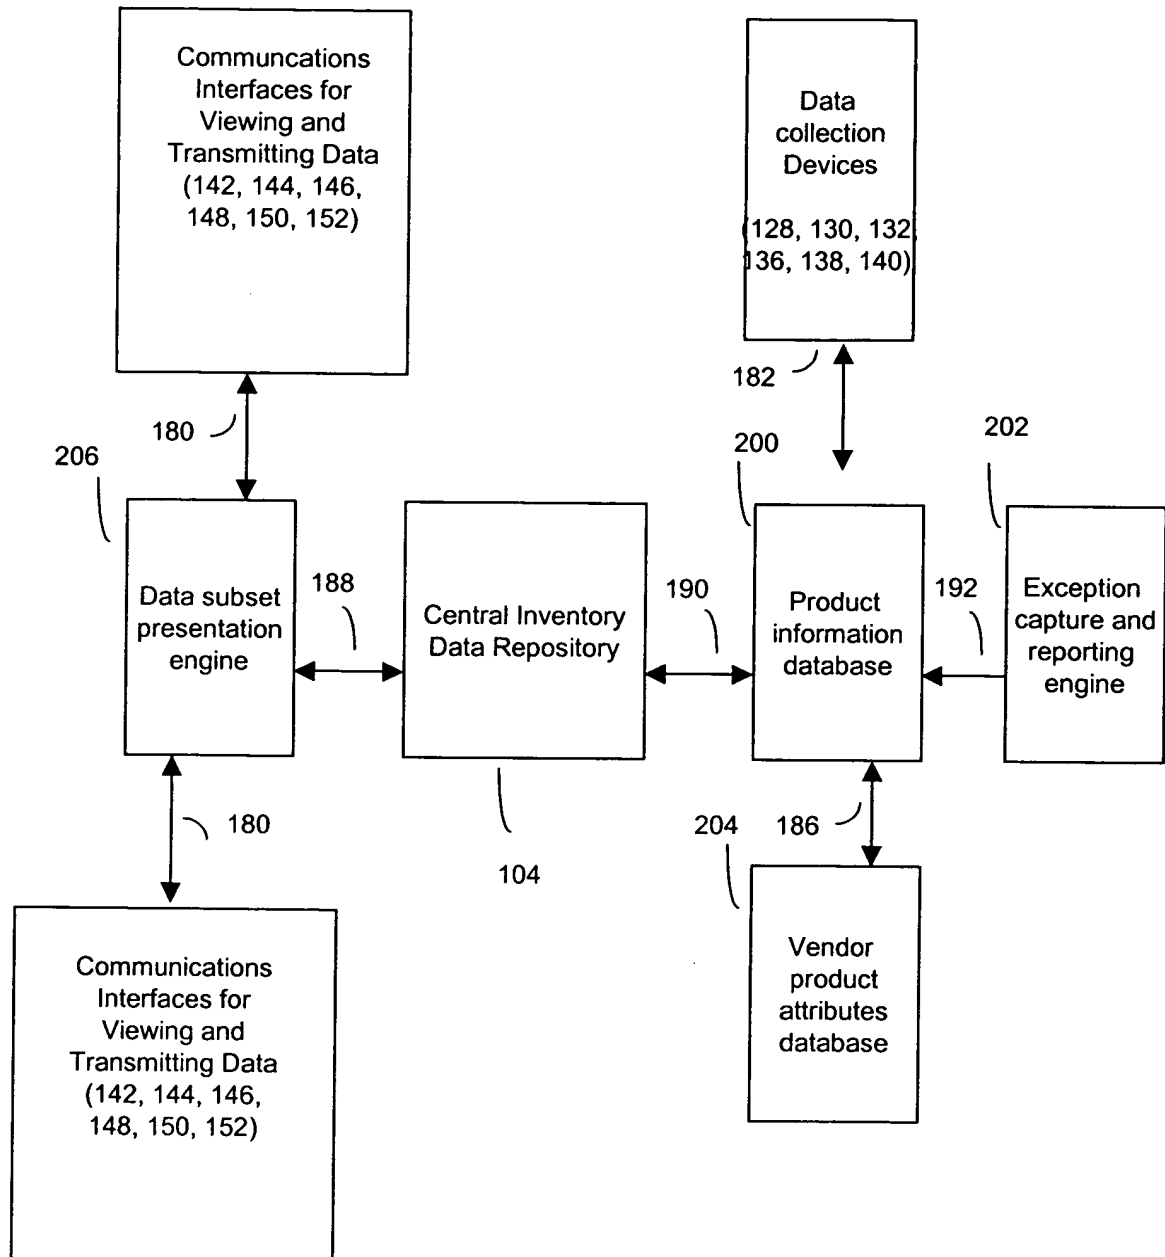
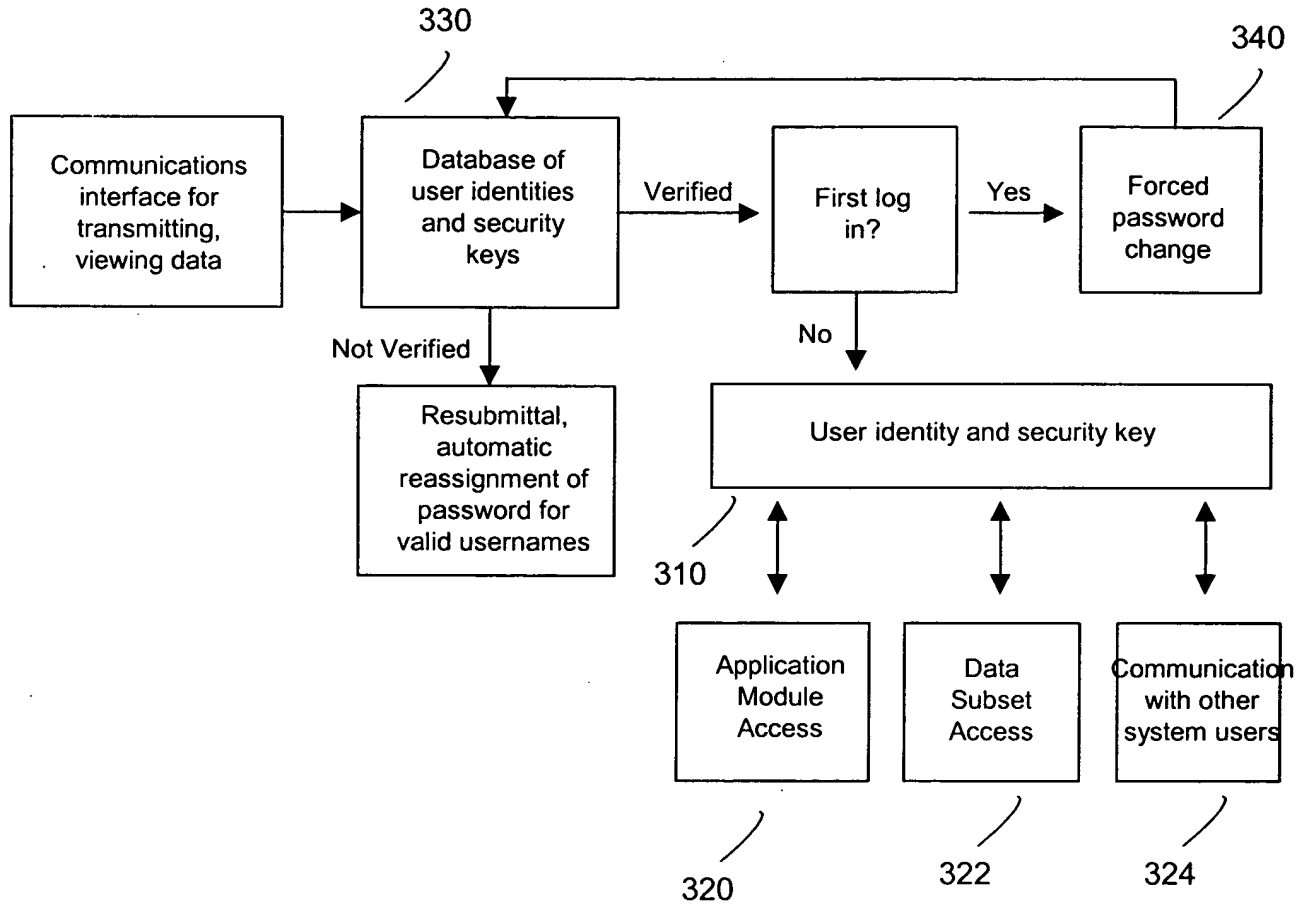
FIG. 3

FIG. 4



40605460 20030403

FIG. 5

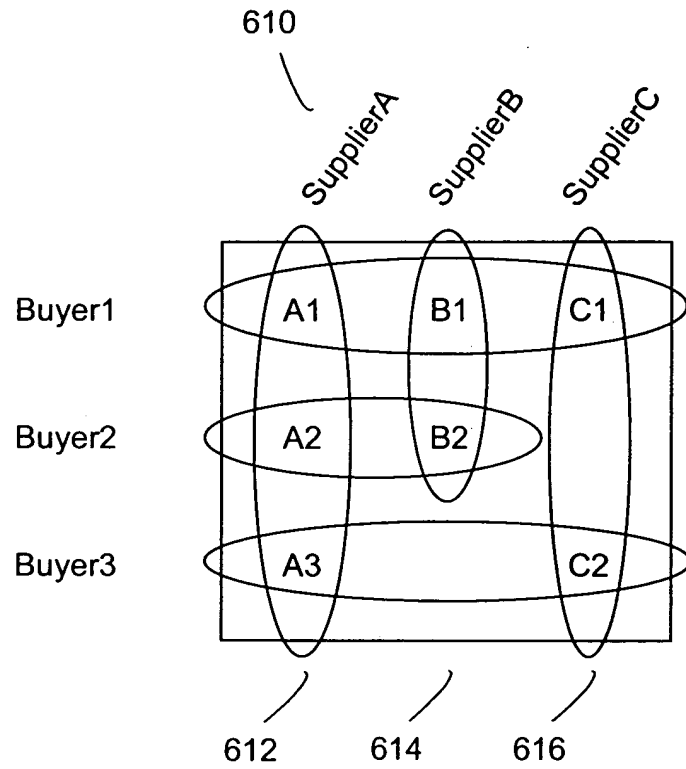


FIG. 6

2-Dimensional Data Table

Username: Regina Hatch

Employer: General Hospital/Interventional Radiology

Tree View

Manufacturer	Accessories	Interve	Balloon Catheter	Catheter	Catheter Ablation	Closure Device
All Manufacturers	146		153	199	5	26
Advanced Medical Designs, Inc.	119	0	0	0	0	0
Allegiance	0	0	0	0	0	0
Arrow International, Inc.	0	0	0	81	0	0
Bard Electrophysiology	0	0	0	0	5	0
Bard Medical	0	0	0	6	0	0
Bard Urological	0	0	0	65	0	0
Biosphere Medical	0	0	0	0	0	0
Boston Scientific/EPT	3	0	0	11	0	0
Boston Scientific/Scimed	0	0	76	0	0	0
Boston Scientific/Target Therapeuti	0	0	0	0	0	0
C.R. Bard, Inc.	0	0	0	14	0	0
Cook Inc.	0	0	0	22	0	0
Cordis, a Johnson & Johnson Comp	0	0	0	0	0	0
DAIG Corporation, a St. Jude Medic	0	0	0	0	0	0
	27	0	0	0	0	0

FIG. 7

“Tree”-form Hierarchical
Data Table

Inventory

Reports

Orders

Encounters

Tools

Username

Reginald Hatch

Employer

General Hospital/Interventional Radiology

Current Inventory

Table View

Expand All

Expand Next

Collapse Next

Collapse All

+

Accessories - Interventional

▢

Balloon Catheter

▢

Boston Scientific/Scimed

▢

MAX

15779 | MODEL 7F MAX T1 55CM

UOM: EA | Qty/UOM: 1 | Qty: 11

15787 | MODEL 7F MAX CL1 40CM

UOM: EA | Qty/UOM: 1 | Qty: 65

+

Cordis, a Johnson & Johnson Company

+

Catheter

▢

Catheter, Ablation

+

Bard Electrophysiology

+

Closure Device

+

Contrast Material

+

Defibrillators & Leads

FIG. 8

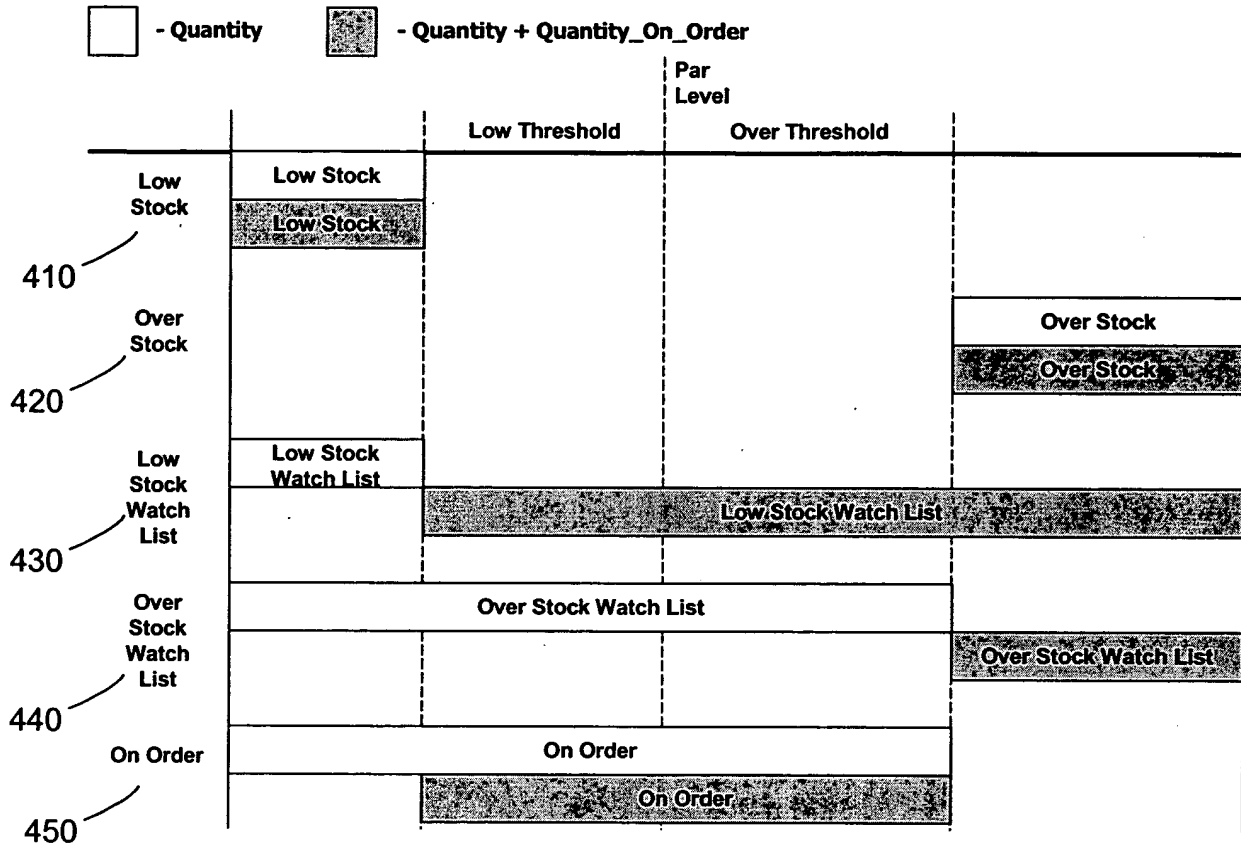
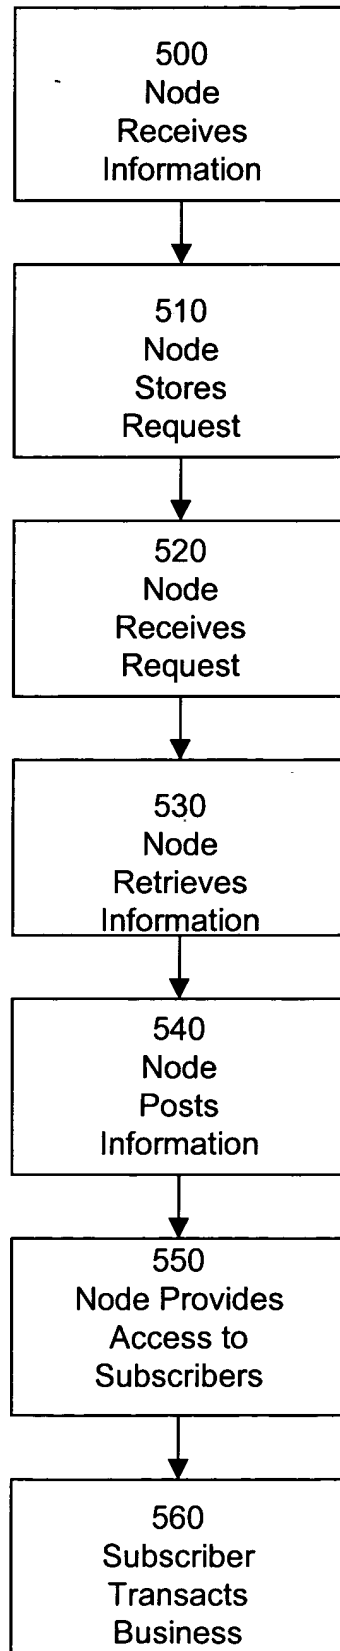


FIG. 9



10050645.044502